



SUB-COMMITTEE ON BULK LIQUIDS
AND GASES
10th session
Agenda item 7

BLG 10/WP.4
5 April 2006
Original: ENGLISH

AMENDMENTS TO RESOLUTION MEPC.2(VI)

Report of the Drafting Group on Sewage Related Issues

Introduction

1 The Drafting Group on Sewage Related Issues met on 4 and 5 April 2006 under the chairmanship of Ms. A. Caston (Australia).

2 The group was attended by delegations from the following Member Governments:

GERMANY
IRELAND
JAPAN

REPUBLIC OF KOREA
UNITED KINGDOM
UNITED STATES

and an observer from the following non-governmental organization:

INTERNATIONAL COUNCIL OF CRUISE LINES (ICCL)

Terms of reference

3 The group, taking into consideration the comments and decisions made in plenary, was instructed to:

- .1 finalize the draft text of the Revised Guidelines on implementation of effluent standards and performance tests for sewage treatment plants to resolution MEPC.2(VI) using the annex to document BLG 10/7 as a basis; and
- .2 submit a written report to plenary on Thursday, 6 April 2006.

Draft text of the proposed Revised Guidelines to resolution MEPC.2(VI)

4 The group, as instructed and taking into consideration comments made in plenary, finalized the draft text of the Revised Guidelines to resolution MEPC.2(VI).

5 In doing so, the group also made several minor editorial changes to the draft text to improve clarity, in particular to paragraphs 3.2, 5.2.2, 5.4.2 and 5.9.5 and section 7. With regard to section 7, a new text was drafted and placed in square brackets for consideration by the Sub-Committee.

For reasons of economy, this document is printed in a limited number. Delegates are kindly asked to bring their copies to meetings and not to request additional copies.

6 The draft text of the Revised Guidelines on implementation of effluent standards and performance tests for sewage treatment plants and the associated draft MEPC resolution are set out at the annex for consideration by the Sub-Committee.

Action requested of the Sub-Committee

7 The Sub-Committee is invited to approve the report in general and in particular to:

- .1 agree the text in section 7 of the Revised Guidelines (paragraph 5 and annex); and
- .2 agree to the draft MEPC resolution on the Revised Guidelines on implementation of effluent standards and performance tests for sewage treatment plants, (paragraph 6 and annex).

ANNEX

**DRAFT RESOLUTION MEPC...(55)
(adopted onOctober 2006)****REVISED GUIDELINES ON IMPLEMENTATION OF EFFLUENT STANDARDS AND
PERFORMANCE TESTS FOR SEWAGE TREATMENT PLANTS**

THE MARINE ENVIRONMENT PROTECTION COMMITTEE,

RECALLING Article 38(a) of the Convention on the International Maritime Organization concerning the functions of the Marine Environment Protection Committee (the Committee) conferred upon it by international conventions for the prevention and control of marine pollution,

NOTING resolution MEPC.2(VI) adopted on 3 December 1976 by which the Marine Environment Protection Committee adopted, at its sixth session, the Recommendation on International Effluent Standards and Guidelines for Performance Tests for Sewage Treatment Plants and invited Governments to apply the Effluent Standards and Guidelines for approving sewage treatment plants; to take steps to establish testing programmes in accordance with the Guidelines for Performance Tests; and provide the Organization with a list of sewage treatment plants meeting the standards,

NOTING ALSO resolution MEPC.115(51) adopted on 1 April 2004 by which the Marine Environment Protection Committee adopted, at its fifty-first session, the revised MARPOL Annex IV and which entered into force on 1 August 2005,

NOTING FURTHER the provisions of regulation 9.1.1 of MARPOL Annex IV, in which reference is made to the above-mentioned guidelines,

RECOGNIZING that resolution MEPC.2(VI) should be amended in order that current trends for the protection of the marine environment and developments in the design and effectiveness of commercially available sewage treatment plants be reflected; and the proliferation of differing unilateral more stringent standards that might be imposed worldwide be avoided,

HAVING CONSIDERED the recommendation made by the Sub-Committee on Bulk Liquids and Gases, at its tenth session,

1. ADOPTS the Revised Guidelines on Implementation of Effluent Standards and Performance Tests for Sewage Treatment Plants, the text of which is set out in the annex to this resolution;
2. INVITES Governments to:
 - (a) implement the Revised Guidelines on Implementation of Effluent Standards and Performance Tests for Sewage Treatment Plants and apply them so that all equipment installed on board on or after [DD/MM/YY] meets the Revised Guidelines in so far as is reasonable and practicable; and

- (b) provide the Organization with information on experiences gained from their application and, in particular, on successful testing of equipment against the Standards;
3. REQUESTS the Secretariat, on the basis of information received, to maintain and update a list of approved equipment and to circulate it once a year to Governments;
4. FURTHER INVITES Governments to issue an appropriate “Certificate of type approval for Sewage Treatment Plants” as referred to in paragraph 5.4.2 and the annex of the Revised Guidelines and to recognize such certificates issued under the authority of other Governments as having the same validity as certificates issued by them; and
5. SUPERSEDES the Recommendation on International Effluent Standards and Guidelines for Performance Tests for Sewage Treatment Plants contained in resolution MEPC.2(VI).

ANNEX

**REVISED GUIDELINES ON IMPLEMENTATION OF EFFLUENT STANDARDS AND
PERFORMANCE TESTS FOR SEWAGE TREATMENT PLANTS**

TABLE OF CONTENTS

- 1 Introduction
- 2 Definitions
- 3 General
- 4 Standards
- 5 Testing considerations
- 6 Renewal and additional surveys
- [7 Familiarization of ship personnel in the use of the sewage treatment plant]

ANNEX

Form of Certificate of Type Approval for Sewage Treatment Plants and Appendix

REVISED GUIDELINES ON IMPLEMENTATION OF EFFLUENT STANDARDS AND PERFORMANCE TESTS FOR SEWAGE TREATMENT PLANTS

1 INTRODUCTION

1.1 The Marine Environment Protection Committee (MEPC) of the International Maritime Organization (IMO) adopted resolution MEPC.2(VI) Recommendation on International Effluent Standards and Guidelines for Performance Tests for Sewage Treatment Plants in 1976.

1.2 This document contains the Revised Guidelines on Implementation of Effluent Standards and Performance Tests for Sewage Treatment Plants (Guidelines). These Guidelines are intended to assist Administrations in establishing operational performance testing programmes for sewage treatment plants for the purpose of type approval under regulation 9.1.1 of Annex IV of the Convention.

1.3 These Guidelines apply to sewage treatment plants fitted to ships, the keel of which was laid or which is at a similar stage of construction on or after [DD/MM/YY].

2 DEFINITIONS

Annex IV – the revised Annex IV of the International Convention for the Prevention of Pollution from Ships (MARPOL 73/78) as amended by resolution MEPC.115(51).

Convention – the International Convention for the Prevention of Pollution from Ships 1973/1978 (MARPOL 73/78).

Geometric mean – the n th root of the product of n numbers.

Greywater – is drainage from dishwater, shower, laundry, bath and washbasin drains.

Testing onboard – testing carried out on a sewage treatment plant that has been installed upon a ship.

Testing ashore – testing carried out on a sewage treatment plant prior to installation e.g. in the factory.

Thermotolerant coliforms – the group of coliform bacteria which produce gas from lactose in 48 hours at 44.5°C. These organisms are sometimes referred to as “faecal coliforms”; however, the term “thermotolerant coliforms” is now accepted as more appropriate, since not all of these organisms are of faecal origin.

3 GENERAL

3.1 An approved sewage treatment plant must meet the standards in section 4 and the tests outlined in these Guidelines. It should also be noted that, when ships are operating approved sewage treatment plants, Annex IV also provides that the effluent shall not produce visible floating solids or cause discolouration of the surrounding water.

3.2 It is acknowledged that the performance of sewage treatment plants may vary considerably when the system is tested ashore under simulated shipboard conditions or onboard a ship under actual operating conditions. Where testing ashore demonstrates that a system complies with the standards, but subsequent onboard testing does not meet the standards, the Administration should determine the reason and take it into account when deciding whether to type approve the plant.

3.3 It is recognized that Administrations may wish to modify the specific details outlined in these Guidelines to take account of very large, very small or unique sewage treatment plants.

4 STANDARDS

4.1 For the purpose of regulation 4.1 of Annex IV, a sewage treatment plant should satisfy the following effluent standards when tested for its Certificate of Type Approval by the Administration:

.1 Thermotolerant Coliform Standard

The geometric mean of the thermotolerant coliform count of the samples of effluent taken during the test period should not exceed 100 thermotolerant coliforms/100 ml as determined by membrane filter, multiple tube fermentation or an equivalent analytical procedure.

.2 Total Suspended Solids Standard

(a) The geometric mean of the total suspended solids content of the samples of effluent taken during the test period shall not exceed 35 mg/l.

(b) Where the sewage treatment plant is tested onboard a ship, the geometric mean of the total suspended solids content of the samples of effluent taken during the test period shall not be more than 70 mg/l above the suspended solids content of ambient water used for flushing purposes.

Analysis for total suspended solids should be conducted in accordance with gravimetric methods approved by the Administration.

.3 Biochemical Oxygen Demand and Chemical Oxygen Demand

Administrations should satisfy themselves that the sewage treatment plant is designed to reduce both soluble and insoluble organic substances to meet the requirement that, the geometric mean of 5-day Biochemical Oxygen Demand (BOD₅) of the samples of effluent taken during the test period does not exceed 25 mg/l and the Chemical Oxygen Demand (COD) does not exceed 125 mg/l. Appropriate methods may include COD Manganese and/or COD Chromium.

.4 pH

The pH of the samples of effluent taken during the test period shall be between 6 and 8.5.

.5 Zero or non-detected values

For thermolerant coliforms, zero values should be replaced with a value of 1 thermotolerant coliform/100 ml to allow the calculation of the geometric mean. For total suspended solids, biochemical oxygen demand and chemical oxygen demand, values below the limit of detection should be replaced with one half the limit of detection to allow the calculation of the geometric mean.

4.2 Where the sewage treatment plant has been tested ashore, the initial survey should include installation and commissioning of the sewage treatment plant.

5 TESTING CONSIDERATIONS

5.1 Testing of the operational performance of a sewage treatment plant should be conducted in accordance with the following subparagraphs. Unless otherwise noted, the subparagraphs apply to testing both onboard and ashore.

5.2 Raw sewage quality

5.2.1 Sewage treatment plants tested ashore - the influent should be fresh sewage consisting of faecal matter, urine, toilet paper and flush water to which, for testing purposes primary sewage sludge has been added as necessary to attain a minimum total suspended solids concentration appropriate for the number of persons and hydraulic loading for which the sewage treatment plant will be certified. The testing should take into account the type of system (for example vacuum or gravity toilets) and any water or greywater that may be added for flushing to the sewage before treatment. In any case the influent concentration of total suspended solids should be no less than 500 mg/l.

5.2.2 Sewage treatment plants tested onboard - the influent may consist of the sewage generated under normal operational conditions. In any case the average influent concentration of total suspended solids should be no less than 500 mg/l.

5.3 Duration and timing of test

5.3.1 The duration of the test period should be a minimum of 10 days and should be timed to capture normal operational conditions, taking into account the type of system and the number of persons and hydraulic loading for which the sewage treatment plant will be type approved. The test should commence after steady-state conditions have been reached by the sewage treatment plant under test.

5.4 Loading factors

5.4.1 During the test period the sewage treatment plant should be tested under conditions of minimum, average and maximum volumetric loadings.

.1 For testing ashore, these loadings will be as laid down in the manufacturer's specifications. Figure 1 shows suggested timings for sampling each loading factor.

- .2 For testing onboard, minimum loading will represent that generated by the number of persons on the ship when it is alongside in port, and average and maximum loadings will represent those generated by the number of persons on the ship at sea and will take account of meal times and watch rotations.

5.4.2 The Administration should undertake to assess the capability of the sewage treatment plant to produce an effluent in accordance with the standards prescribed by section 4 following minimum, average and maximum volumetric loadings. The range of conditions under which the effluent standards were met should be recorded on the Certificate of Type Approval. The form of the Certificate of Type Approval and appendix is set out in the annex to these Guidelines.

5.5 Sampling methods and frequency

5.5.1 Administrations should ensure that the sewage treatment plant is installed in a manner which facilitates the collection of samples. Sampling should be carried out in a manner and at a frequency which is representative of the effluent quality. Figure 1 provides a suggested frequency for sampling, however, the frequency should take account of the residence time of the influent in the sewage treatment plant. A minimum of 40 effluent samples should be collected to allow a statistical analysis of the testing data (e.g. geometric mean, maximum, minimum, variance).

5.5.2 An influent sample should be taken and analyzed for every effluent sample taken and the results recorded to ensure compliance with section 4. If possible, additional influent and effluent samples should be taken to allow for a margin of error. Samples should be appropriately preserved prior to analysis particularly if there is to be a significant delay between collection and analysis or during times of high ambient temperature.

5.5.3 Any disinfectant residual in samples should be neutralized when the sample is collected to prevent unrealistic bacteria kill or chemical oxidation of organic matter by the disinfectant brought about by artificially extended contact times. Chlorine (if used) concentration and pH should be measured prior to neutralization.

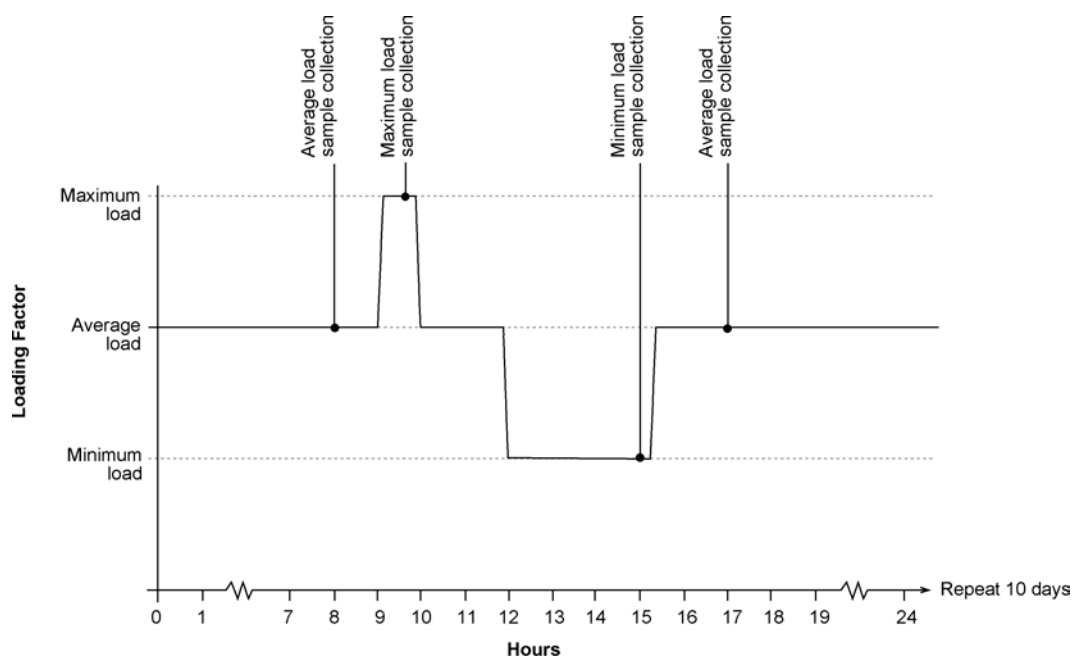


Figure 1: Suggested hydraulic loading factors and sampling frequency for testing sewage treatment plants. May be modified as necessary to take account of characteristics of individual sewage treatment plants.

5.6 Analytical testing of effluent

5.6.1 The Administration should give consideration to the recording of other parameters in addition to those required (thermotolerant coliforms, total suspended solids, BOD₅, COD, pH and residual chlorine) with a view to future technological development. Parameters which might be considered include total solids, volatile solids, settleable solids, volatile suspended solids, turbidity, total phosphorus, total organic carbon, total coliforms and faecal streptococci.

5.7 Disinfectant residual

5.7.1 The potential adverse environmental effects of many disinfectant residuals and by-products, such as those associated with the use of chlorine or its compounds, are well recognized. It is, therefore, recommended that Administrations encourage the use of ozone, ultra-violet irradiation or any other disinfectants which minimize adverse environmental effects, whilst pursuing the thermotolerant coliform standard. When chlorine is used as a disinfectant, the Administration should be satisfied that the best technical practice is used to keep the disinfectant residual in the effluent below [0.1][0.5][2.5] mg/l.

5.8 Scaling considerations

5.8.1 Only full-scale marine sewage treatment plants should be accepted for testing purposes. The Administration may certify a range of the manufacturer's equipment sizes employing the same principles and technology, but due consideration must be given to limitations on performance which might arise from scaling up or scaling down. In the case of very large, very small or unique sewage treatment plants, certification may be based on results of prototype tests. Where possible, confirmatory tests should be performed on the final installation of such sewage treatment plants.

5.9 Environmental testing of the sewage treatment plant

5.9.1 The Administration should be satisfied that the sewage treatment plant can operate under conditions of tilt consistent with internationally acceptable shipboard practice.

5.9.2 Tests for certification should be carried out over the range of temperature and salinity specified by the manufacturer, and the Administration should be satisfied that such specifications are adequate for the conditions under which the equipment must operate.

5.9.3 Control and sensor components should be subjected to environmental testing to verify their suitability for marine use. The Test Specifications section in part 3 of the annex to resolution MEPC.107(49) provides guidance in this respect.

5.9.4 Any limitation on the conditions of operation should be recorded on the Certificate.

5.9.5 The Administration should also consider requiring the manufacturer to include in the operating and maintenance manuals, a list of chemicals and materials suitable for use in the operation of the sewage treatment plant.

5.10 Other considerations

5.10.1 The type and model of the sewage treatment plant and the name of the manufacturer should be noted by means of a durable label firmly affixed directly to the sewage treatment plant. This label should include the date of manufacture and any operational or installation limits considered necessary by the manufacturer or the Administration.

5.10.2 Administrations should examine the manufacturer's installation, operating and maintenance manuals for adequacy and completeness. The ship should have on board at all times a manual detailing the operational and maintenance procedures for the sewage treatment plant.

5.10.3 Qualifications of testing facilities should be carefully examined by the Administration as a prerequisite to their participation in the testing programme. Every attempt should be made to assure uniformity among the various facilities.

6 RENEWAL AND ADDITIONAL SURVEYS

6.1 Administrations should endeavour to ensure, when conducting renewal or additional surveys in accordance with regulations 4.1.2 and 4.1.3 of Annex IV, that the sewage treatment plant continues to perform in accordance with the conditions outlined in regulation 4.1.1 of Annex IV.

7 FAMILIARIZATION OF SHIP PERSONNEL IN THE USE OF THE SEWAGE TREATMENT PLANT

[7.1 Recognizing that the appropriate regulations relating to familiarization are contained within the Ships Safety Management Systems under the International Safety Management Code, Administrations are reminded that ship staff training should include familiarization in the operation and maintenance of the sewage treatment plant.]

ANNEX

FORM OF CERTIFICATE OF TYPE APPROVAL
FOR SEWAGE TREATMENT PLANTS AND APPENDIX

BADGE
OR
CIPHER

NAME OF ADMINISTRATION

**CERTIFICATE OF TYPE APPROVAL
FOR SEWAGE TREATMENT PLANTS**

This is to certify that the Sewage Treatment Plant, Type.....,
having a designed hydraulic loading of cubic metres per day, (m³/day), an organic loading of
..... kg per day Biochemical Oxygen Demand (BOD) and of the design shown on Drawings Nos.
manufactured by

has been examined and satisfactorily tested in accordance with the International Maritime Organization
resolution MEPC.[](55) to meet the operational requirements referred to in regulation 9.1.1 of Annex IV
of the International Convention for the Prevention of Pollution from Ships, 1973/78 as modified by
resolution MEPC.115(51).

The tests on the sewage treatment plant were carried out
ashore at*
onboard at*
and completed on

The sewage treatment plant was tested and produced an effluent which, on analysis, produces:

- (i) a geometric mean of no more than 100 thermotolerant coliforms/100 ml;
- (ii) a geometric mean of total suspended solids of 35 mg/l if tested ashore or a geometric mean of total suspended solids of 70 mg/l above the ambient water used for flushing purposes if tested onboard;
- (iii) a geometric mean of 5-day Biochemical Oxygen Demand (BOD₅) of no more than 25 mg/l;
- (iv) a geometric mean of Chemical Oxygen Demand of no more than 125 mg/l;
- (v) pH of the effluent is between 6 and 8.5.

The Administration is satisfied that the sewage treatment plant can operate at angles of inclination of 22.5° in any plane from the normal operating position.

Details of the tests and the results obtained are shown on the Appendix to this Certificate.

A plate or durable label containing data of the manufacturer's name, type and serial numbers, hydraulic loading and date of manufacture is to be fitted on each sewage treatment plant.

A copy of this Certificate shall be carried on board any ship equipped with the above described sewage treatment plant.

Official stamp Signed

Administration of

Dated this.....day.....of.....20....

* Delete as appropriate.

BADGE
OR
CIPHER

APPENDIX TO
CERTIFICATE OF TYPE APPROVAL FOR SEWAGE TREATMENT PLANTS

Test results and details of tests conducted on samples from the Sewage Treatment Plant in accordance with resolution MEPC.[...](55):

Sewage Treatment Plant, Type
 Manufactured by
 Organization conducting the test
 Designed hydraulic loading m³/day
 Designed organic loading kg/day BOD

Number of effluent samples tested
 Number of influent samples tested
 Raw sewage (influent) quality mg/l Total Suspended Solids
 Maximum hydraulic loading m³/day
 Minimum hydraulic loading m³/day
 Average hydraulic loading m³/day

Geometric Mean of Total
 Suspended Solids mg/l
 Geometric Mean of the thermotolerant
 coliform count coliforms/100 ml
 Geometric Mean of BOD₅ mg/l

Type of disinfectant used
 If Chlorine - residual Chlorine:
 Maximum mg/l
 Minimum mg/l
 Geometric Mean mg/l

Was the sewage treatment plant tested with:
 Fresh Water flushing? Yes/No*
 Salt Water flushing? Yes/No*
 Fresh and Salt Water flushing? Yes/No*
 Greywater added? Yes – proportion: /No*

Was the sewage treatment plant tested against the environmental conditions specified in section 5.9 of resolution MEPC.[...](55):
 Temperature Yes/No*
 Humidity Yes/No*
 Inclination Yes/No*
 Vibration Yes/No*
 Reliability of Electrical and Electronic Equipment Yes/No*

Limitations and the conditions of operation are imposed:
 Salinity
 Temperature
 Humidity
 Inclination
 Vibration

Results of other parameters tested
 Official stamp Signed
 Administration of Dated this day of 20

* Delete as appropriate.